

## USER GUIDE

# NI Vision I/O Terminal Block and Prototyping Accessory

This document describes the features of your NI Vision I/O Terminal Block and Prototyping Accessory, what you need to get started, and the installation and operation of the device.

## Introduction

---

The NI Vision I/O Accessory breaks out the I/O functionality of the NI CVS-1450 Series compact vision system, NI PCI-8254R, and the NI PCIe-8255R, providing screw terminals for easy connections. The NI Vision I/O Accessory also provides LEDs for each signal, which you can use to quickly prototype and troubleshoot your application.

You can use the NI Vision I/O Accessory in demo mode or user mode. Demo mode allows you to quickly prototype your application, and user mode allows you to debug a deployed application.

## What You Need to Get Started

---

- NI Vision I/O Terminal Block and Prototyping Accessory
- One of the following image acquisition devices:
  - NI CVS-1450 Series compact vision system
  - NI PCI-8254R
  - NI PCIe-8255R
- Vision Builder for Automated Inspection (Vision Builder AI) script or LabVIEW VI to run on the CVS-1450 device, NI 8254R, or NI 8255R device

## Related Documentation

The following documents contain information you may find helpful as you set up and use the NI Vision I/O Accessory:

- *NI CVS-1450 Series User Manual*—Describes how to set up and configure the CVS-1450 device to acquire and display an initial image. This document also contains hardware specifications, troubleshooting guidelines, and information about the LEDs, DIP switches, and connectors on the CVS-1450 device.
- *NI 1450 Series Compact Vision System Quick Start Guide*—Describes how to set up and configure the NI 1450 Series device to acquire an image using either NI Vision Builder for Automated Inspection or the LabVIEW Real-Time Module. This document also provides instructions for configuring an IP address and verifying that hardware and software are properly installed.
- *NI PCI-8254 Quick Start Guide*—Contains important safety information; wiring information; specifications; and information about unpacking, installing, and configuring the NI PCI-8254R.
- *NI PCI-8254 User Manual*—Contains software and hardware overviews for the NI PCI-8254R, and provides I/O reference material.
- *NI PCIe-8255 Quick Start Guide*—Contains important safety information; wiring information; specifications; and information about unpacking, installing, and configuring the NI PCIe-8255R.
- *NI PCIe-8255 User Manual*—Contains software and hardware overviews for the NI PCIe-8255R, and provides I/O reference material.

## Safety Information

---



**Caution** The following paragraphs contain important safety information you *must* follow when installing and operating the device.

Do *not* operate the device in a manner not specified in the documentation. Misuse of the device may result in a hazard and may compromise the safety protection built into the device. If the device is damaged, turn it off and do *not* use it until service-trained personnel can check its safety. If necessary, return the device to National Instruments for repair.

Keep away from live circuits. Do *not* remove equipment covers or shields unless you are trained to do so. If signal wires are connected to the device, hazardous voltages can exist even when the equipment is turned off. To avoid a shock hazard, do *not* perform procedures involving cover or shield removal unless you are qualified to do so. Disconnect all field power prior to removing covers or shields.

If the device is rated for use with hazardous voltages ( $>30 V_{\text{rms}}$ ,  $42.4 V_{\text{pk}}$ , or  $60 V_{\text{dc}}$ ), it may require a safety earth-ground connection wire. Refer to the device specifications for maximum voltage ratings.

Because of the danger of introducing additional hazards, do *not* install unauthorized parts or modify the device. Use the device only with the chassis, modules, accessories, and cables specified in the installation instructions. All covers and filler panels *must* be installed while operating the device.

Do *not* operate the device in an explosive atmosphere or where flammable gases or fumes may be present. Operate the device only at or below the pollution degree stated in the specifications. Pollution consists of any foreign matter—solid, liquid, or gas—that may reduce dielectric strength or surface resistivity. The following is a description of pollution degrees.

- Pollution Degree 1—No pollution or only dry, nonconductive pollution occurs. The pollution has no effect.
- Pollution Degree 2—Normally only nonconductive pollution occurs. Occasionally, nonconductive pollution becomes conductive because of condensation.
- Pollution Degree 3—Conductive pollution or dry, nonconductive pollution occurs. Nonconductive pollution becomes conductive because of condensation.

Clean the device and accessories by brushing off light dust with a soft, nonmetallic brush. Remove other contaminants with a stiff, nonmetallic brush. The unit *must* be completely dry and free from contaminants before returning it to service.

You *must* insulate signal connections for the maximum voltage for which the device is rated. Do *not* exceed the maximum ratings for the device. Remove power from signal lines before connection to or disconnection from the device.



**Caution** National Instruments measurement products may be classified as either Measurement Category I or II. Operate products at or below the Measurement Category level specified in the hardware specifications.

**Measurement Category**<sup>1</sup>: Measurement circuits are subjected to working voltages<sup>2</sup> and transient stresses (overvoltage) from the circuit to which they are connected during measurement or test. Measurement Category establishes standardized impulse withstand voltage levels that commonly

---

<sup>1</sup> Measurement Categories as defined in electrical safety standard IEC 61010-1.

<sup>2</sup> Working voltage is the highest rms value of an AC or DC voltage that can occur across any particular insulation.

occur in electrical distribution systems. The following is a description of Measurement (Installation<sup>1</sup>) Categories:

- Measurement Category I is for measurements performed on circuits *not* directly connected to the electrical distribution system referred to as MAINS<sup>2</sup> voltage. This category is for measurements of voltages from specially protected secondary circuits. Such voltage measurements include signal levels, special equipment, limited-energy parts of equipment, circuits powered by regulated low-voltage sources, and electronics.
- Measurement Category II is for measurements performed on circuits directly connected to the electrical distribution system. This category refers to local-level electrical distribution, such as that provided by a standard wall outlet (e.g., 115 V for U.S. or 230 V for Europe). Examples of Measurement Category II are measurements performed on household appliances, portable tools, and similar products.
- Measurement Category III is for measurements performed in the building installation at the distribution level. This category refers to measurements on hard-wired equipment such as equipment in fixed installations, distribution boards, and circuit breakers. Other examples are wiring, including cables, bus-bars, junction boxes, switches, socket-outlets in the fixed installation, and stationary motors with permanent connections to fixed installations.
- Measurement Category IV is for measurements performed at the primary electrical supply installation (<1,000 V). Examples include electricity meters and measurements on primary overcurrent protection devices and on ripple control units.

## Compliance with FCC/Canada Radio Frequency Interference Regulations

---

### Determining FCC Class

The Federal Communications Commission (FCC) has rules to protect wireless communications from interference. The FCC places digital electronics into two classes. These classes are known as Class A (for use in industrial-commercial locations only) or Class B (for use in residential or commercial locations). All National Instruments (NI) products are FCC Class A products.

---

<sup>1</sup> Measurement Category is also referred to as Installation Category.

<sup>2</sup> MAINS is defined as the (hazardous live) electrical supply system to which equipment is designed to be connected for the purpose of powering the equipment. Suitably rated measuring circuits may be connected to the MAINS for measuring purposes.

Depending on where it is operated, this Class A product could be subject to restrictions in the FCC rules. (In Canada, the Department of Communications (DOC), of Industry Canada, regulates wireless interference in much the same way.) Digital electronics emit weak signals during normal operation that can affect radio, television, or other wireless products.

All Class A products display a simple warning statement of one paragraph in length regarding interference and undesired operation. The FCC rules have restrictions regarding the locations where FCC Class A products can be operated.

Consult the FCC Web site at [www.fcc.gov](http://www.fcc.gov) for more information.

## **FCC/DOC Warnings**

This equipment generates and uses radio frequency energy and, if not installed and used in strict accordance with the instructions in this manual and the CE marking Declaration of Conformity<sup>1</sup>, may cause interference to radio and television reception. Classification requirements are the same for the Federal Communications Commission (FCC) and the Canadian Department of Communications (DOC).

Changes or modifications not expressly approved by NI could void the user's authority to operate the equipment under the FCC Rules.

## **Class A**

### **Federal Communications Commission**

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user is required to correct the interference at their own expense.

### **Canadian Department of Communications**

This Class A digital apparatus meets all requirements of the Canadian Interference-Causing Equipment Regulations.

---

<sup>1</sup> The CE marking Declaration of Conformity contains important supplementary information and instructions for the user or installer.

Cet appareil numérique de la classe A respecte toutes les exigences du Règlement sur le matériel brouilleur du Canada.

## Compliance with EU Directives

Users in the European Union (EU) should refer to the Declaration of Conformity (DoC) for information<sup>1</sup> pertaining to the CE marking. Refer to the Declaration of Conformity (DoC) for this product for any additional regulatory compliance information. To obtain the DoC for this product, visit [ni.com/certification](http://ni.com/certification), search by model number or product line, and click the appropriate link in the Certification column.

## Unpacking

---

The NI Vision I/O Accessory ships in an antistatic package to prevent electrostatic discharge from damaging device components. To avoid such damage in handling the device, take the following precautions:

- Ground yourself using a grounding strap or by holding a grounded object.
- Touch the antistatic package to a metal grounded object before removing the device from the package.



**Caution** *Never* touch the exposed pins of connectors.

Remove the device from the package and inspect it for loose components or any other signs of damage. Notify National Instruments if the device appears damaged in any way. Do *not* use a damaged device.

Store the NI Vision I/O Accessory in the antistatic envelope when not in use.

## Installation

---

Complete the following steps to install the NI Vision I/O Accessory:

1. Install the image acquisition device and required software as described in the device manual. Refer to the [Related Documentation](#) section to determine which manuals contain installation information.
2. Use the Digital I/O cable to connect the image acquisition device to the NI Vision I/O Accessory.


---

<sup>1</sup> The CE marking Declaration of Conformity contains important supplementary information and instructions for the user or installer.

# Device Overview

The following sections describe the features of the NI Vision I/O Accessory and instructions for how to use the device in demo mode and user mode.

Figure 1 illustrates the front panel of the NI Vision I/O Accessory.

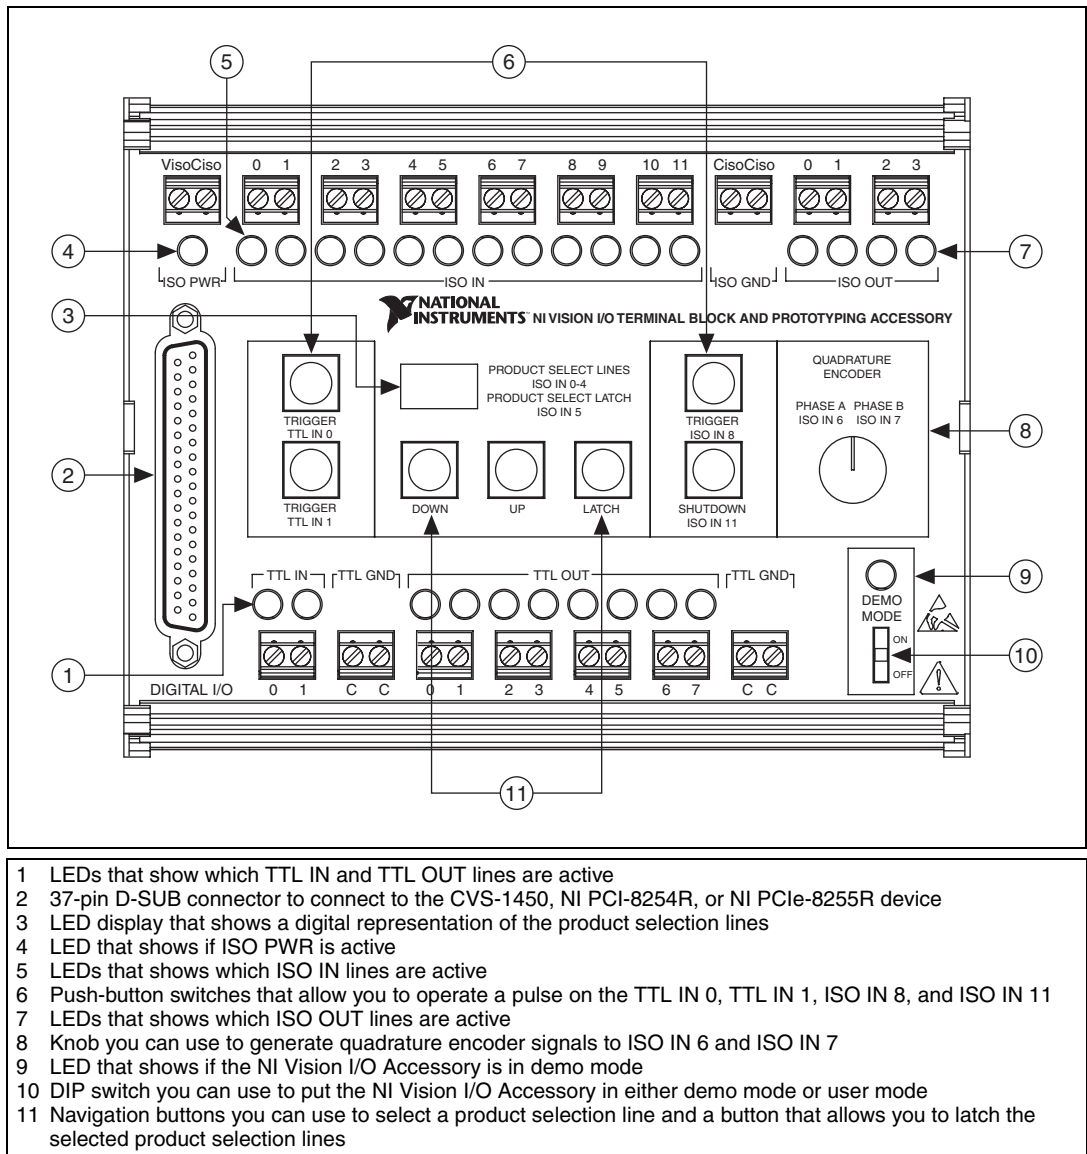

**Figure 1.** NI Vision I/O Accessory Front Panel

## TTL and ISO LED Indicators and Product Selection Display

Each I/O line on the NI Vision I/O Accessory is connected to an LED, which provides quick status information. Each LED lights up when the associated signal is high. This functionality can be useful both for prototyping your image acquisition device solution, as well as for troubleshooting your deployed application. The LEDs function the same way in both demo and user mode.

You typically use product select lines when you have configured your system to perform multiple inspections with one image acquisition device, and the system must switch among the inspections on the fly. The following list includes the ISO lines that are used for product selection:

- ISO IN 0
- ISO IN 1
- ISO IN 2
- ISO IN 3
- ISO IN 4
- ISO IN 5—latch line

The product selection LED display operates differently between demo and user mode. In demo mode, the display provides the decimal representation of the product selection based on the push button switches. In user mode, the display provides the decimal representation for the physical state of the isolated inputs lines that correspond to the product selection port. The latch input, ISO IN 5, is not used when displaying the product selection value.

## Trigger, Shutdown, and Product Select Line Push-button Switches

The NI Vision I/O Accessory provides push-button switches to enable quick development, prototyping, and debugging. You can use the push-button switches to mimic events, such as a trigger from a proximity sensor, an emergency stop signal to shut down the system, or a change to the product selection lines from a programmable logic controller (PLC). When you push the push-button switches, they generate an active-low signal to the image acquisition device. Table 1 shows which signals are connected to the push-button switches.

**Table 1.** Signals with Push-Button Connectivity

Signal Name	Primary Function
TTL Input 1	Trigger Input
TTL Input 2	Trigger Input
ISO Input 8	Trigger Input

**Table 1.** Signals with Push-Button Connectivity (Continued)

Signal Name	Primary Function
ISO Input 11	User Shutdown
ISO Input 0	Product Selection Port, Data (0)
ISO Input 1	Product Selection Port, Data (1)
ISO Input 2	Product Selection Port, Data (2)
ISO Input 3	Product Selection Port, Data (3)
ISO Input 4	Product Selection Port, Data (4)
ISO Input 5	Product Selection Port, Data (5) rising edge latch




**Note** The push-button switches are disabled when the NI Vision I/O Accessory is in user mode.

## Quadrature Encoder

The NI Vision I/O Accessory can demonstrate the use of the quadrature encoder counting capability of the image acquisition device. The accessory provides a 24-pulse per revolution quadrature encoder generator.

The quadrature encoder pulse trains are generated corresponding to the shaft position as you rotate the knob. Depending on the direction of the rotation, phase A leads phase B by 90 or phase B leads phase A by 90. This relationship is illustrated in Figure 2.

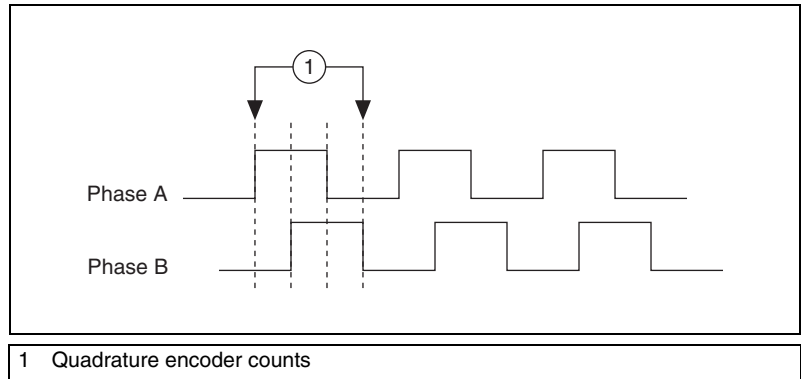

**Figure 2.** Quadrature Encoder Pulse Trains



**Note** The quadrature encoder knob is disabled when the NI Vision I/O Accessory is in user mode.

## DIP Switch


Use the DIP switch on the NI Vision I/O Accessory to determine which mode the accessory is in. The demo mode LED lights when the NI Vision I/O Accessory is in demo mode.

## Using the NI Vision I/O Accessory

---

You can use the NI Vision I/O Accessory in either demo mode or user mode.

### Demo Mode




To use the NI Vision I/O Accessory in demo mode, move the DEMO MODE DIP switch to the ON position. The LED lights up when the NI Vision I/O Accessory is in demo mode.

Use the trigger and product selection push-button switches and the product selection display LED to prototype possible scenarios on the image acquisition device. For example, if you want to prototype a CVS-1450 device application that inspects two different types of products, you can use the product selection push-button switches to toggle between inspections. You also can use the product selection display LED and the ISO IN LEDs to determine which product selection line is currently active.

While the NI Vision I/O Accessory is in demo mode, you can use the ISO and TTL LEDs to observe when the associated signals are high.

Use the quadrature encoder to test the triggering functionality of the image acquisition device for applications that require triggering at a particular position rather than a time. For example, if you want to trigger an image acquisition every few counts, use the quadrature encoder knob to get a feel for how those image acquisitions are triggered.

### User Mode



To use the NI Vision I/O Accessory in user mode, move the DEMO MODE DIP switch to the OFF position.

Use the various TTL and ISO LEDs to view the state of all knobs and trigger lines to allow easy troubleshooting. For example, you can use the TTL OUT LEDs to view which TTL lines are currently triggering other devices.

Use the product selection display LED to view which product selection is currently active.



**Note** The product selection push-button switches are unavailable in user mode.



**Note** The quadrature encoder is unavailable in user mode.

## V<sub>iso</sub> and C<sub>iso</sub>



Use V<sub>iso</sub> and C<sub>iso</sub> to access the isolated power and common mode (ground) signals. If you are using a CVS-1450 device or the NI 8254R device, the power connector on the device provides V<sub>iso</sub> and C<sub>iso</sub>. The CVS-1450 device and the NI 8254R device power the NI Vision I/O Accessory via the 44-pin D-SUB connector.

If you are using the NI 8255R device, the NI Vision I/O Accessory powers the NI 8255R via the 44-pin D-SUB connector. You must provide V<sub>iso</sub> and C<sub>iso</sub> via the V<sub>iso</sub> and C<sub>iso</sub> screw terminals on the NI Vision I/O Accessory. To provide V<sub>iso</sub> and C<sub>iso</sub>, you must connect the NI Vision I/O Accessory to an external power supply. Refer to the *NI PCIe-8255R Quick Start Guide* for more information about connecting an external power supply to the NI Vision I/O Accessory.

## Specifications

---

This section lists the specifications of the NI Vision I/O Accessory. These specifications are typical at 25 °C, unless otherwise noted.

### Power Requirement

Main supply voltage..... 24 VDC ±10%

Power (excluding  
V<sub>iso</sub> and C<sub>iso</sub> connections) ..... 5 W max



**Note** If you are using a CVS-1450 device or the NI 8254R device, power is supplied to the NI Vision I/O Accessory via the 44-pin D-SUB cable connected to the CVS-1450 device or the NI 8254R device.



**Note** If you are using the NI 8255R device, power is supplied to the NI Vision I/O Accessory via the V<sub>iso</sub> and C<sub>iso</sub> screw terminals.

### Physical

Box dimensions (including feet)..... 6.34 in. × 5 in. × 2 in.

Weight..... 10 oz

## Environmental

Operating temperature .....	0 to 55 °C
Storage temperature .....	-20 to 70 °C
Humidity .....	10 to 90%, noncondensing
Maximum altitude.....	2,000 m
Pollution Degree .....	2

The NI Vision I/O Accessory is intended for indoor use only.

## Safety

The NI Vision I/O Accessory is designed to meet the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- EN 61010-1, IEC 61010-1
- UL 61010-1, CAN/CSA-C22.2 No. 61010-1



**Note** For UL and other safety considerations, refer to the product label, or visit [ni.com/certification](http://ni.com/certification), search by model number or product line, and click the appropriate link in the Certification column.

## Electromagnetic Compatibility

The NI Vision I/O Accessory is designed to meet the requirements of the following standards of EMC for electrical equipment for measurement, control, and laboratory use:

- EN 61326 EMC requirements; Minimum Immunity
- EN 55011 Emissions; Group 1, Class A
- CE, C-Tick, ICES, and FCC Part 15 Emissions; Class A



**Note** For EMC compliance, operate this device with shielded cabling.

## CE Compliance

The NI Vision I/O Accessory meets the essential requirements of applicable European Directives, as amended for CE marking, as follows:

- 73/23/EEC; Low-Voltage Directive (safety)
- 89/336/EEC; Electromagnetic Compatibility Directive (EMC)



**Note** Refer to the Declaration of Conformity (DoC) for this product for any additional regulatory compliance information. To obtain the DoC for this product, visit [ni.com/certification](http://ni.com/certification), search by model number or product line, and click the appropriate link in the Certification column.

## Waste Electrical and Electronic Equipment (WEEE)



**EU Customers** At the end of their life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers and National Instruments WEEE initiatives, visit [ni.com/environment/weee.htm](http://ni.com/environment/weee.htm).

## Where to Go for Support

---

The National Instruments Web site is your complete resource for technical support. At [ni.com/support](http://ni.com/support) you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

A Declaration of Conformity (DoC) is our claim of compliance with the Council of the European Communities using the manufacturer's declaration of conformity. This system affords the user protection for electronic compatibility (EMC) and product safety. You can obtain the DoC for your product by visiting [ni.com/certification](http://ni.com/certification). If your product supports calibration, you can obtain the calibration certificate for your product at [ni.com/calibration](http://ni.com/calibration).

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world to help address your support needs. For telephone support in the United States, create your service request at [ni.com/support](http://ni.com/support) and follow the calling instructions or dial 512 795 8248. For telephone support outside the United States, contact your local branch office:

Australia 1800 300 800, Austria 43 0 662 45 79 90 0,  
Belgium 32 0 2 757 00 20, Brazil 55 11 3262 3599,  
Canada 800 433 3488, China 86 21 6555 7838,  
Czech Republic 420 224 235 774, Denmark 45 45 76 26 00,  
Finland 385 0 9 725 725 11, France 33 0 1 48 14 24 24,  
Germany 49 0 89 741 31 30, India 91 80 41190000,  
Israel 972 0 3 6393737, Italy 39 02 413091, Japan 81 3 5472 2970,  
Korea 82 02 3451 3400, Lebanon 961 0 1 33 28 28,  
Malaysia 1800 887710, Mexico 01 800 010 0793,  
Netherlands 31 0 348 433 466, New Zealand 0800 553 322,  
Norway 47 0 66 90 76 60, Poland 48 22 3390150,  
Portugal 351 210 311 210, Russia 7 095 783 68 51,

Singapore 1800 226 5886, Slovenia 386 3 425 4200,  
South Africa 27 0 11 805 8197, Spain 34 91 640 0085,  
Sweden 46 0 8 587 895 00, Switzerland 41 56 200 51 51,  
Taiwan 886 02 2377 2222, Thailand 662 278 6777,  
United Kingdom 44 0 1635 523545

National Instruments, NI, ni.com, and LabVIEW are trademarks of National Instruments Corporation. Refer to the *Terms of Use* section on [ni.com/legal](http://ni.com/legal) for more information about National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your CD, or [ni.com/patents](http://ni.com/patents).